Checking the Orthosis' Alignment

FIOR & GENTZ

1.

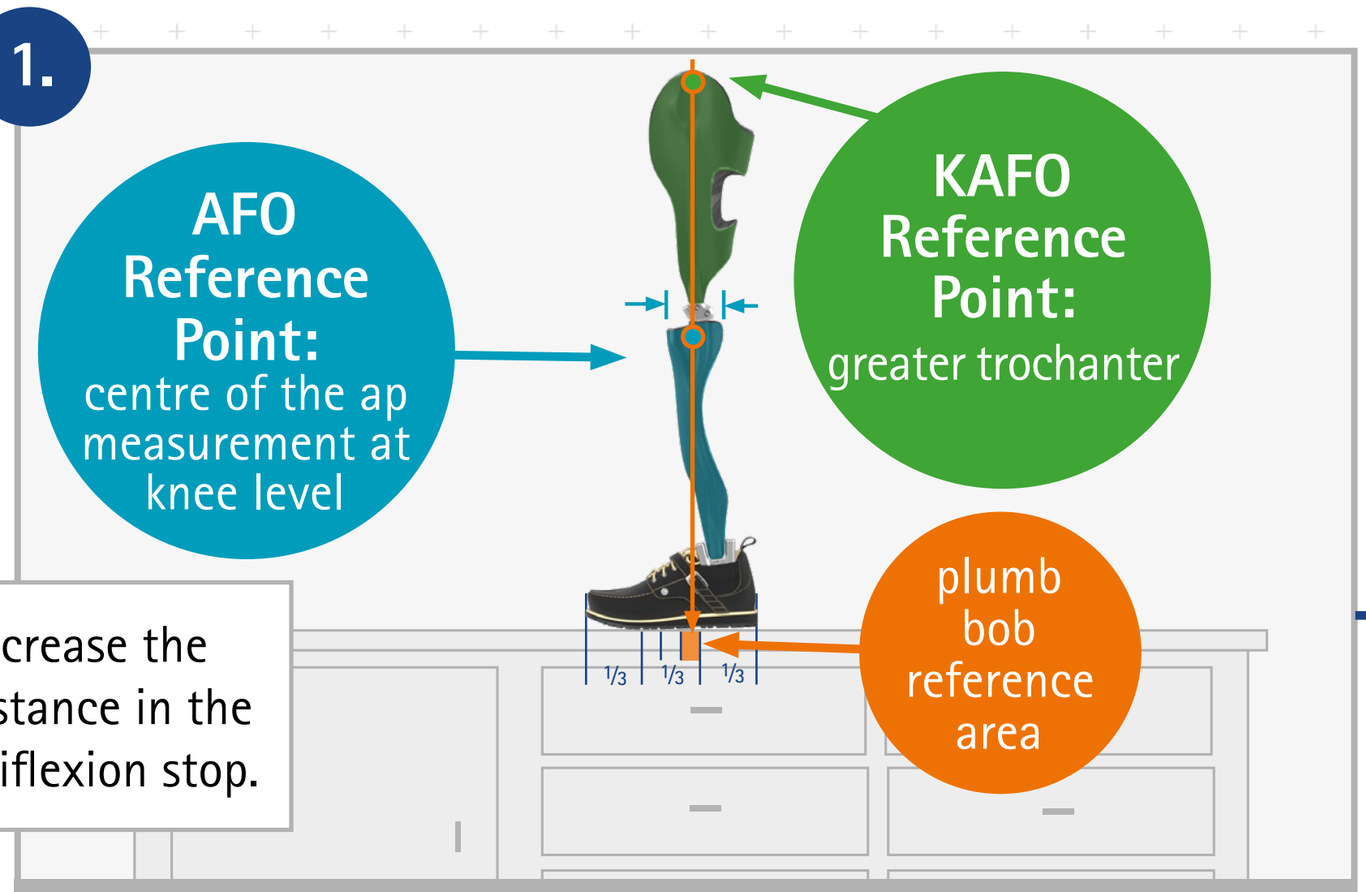

adjusting the orthosis' alignment on the workbench

Increase the resistance in the dorsiflexion stop.

After adjusting the alignment, proceed with step 2.

2.

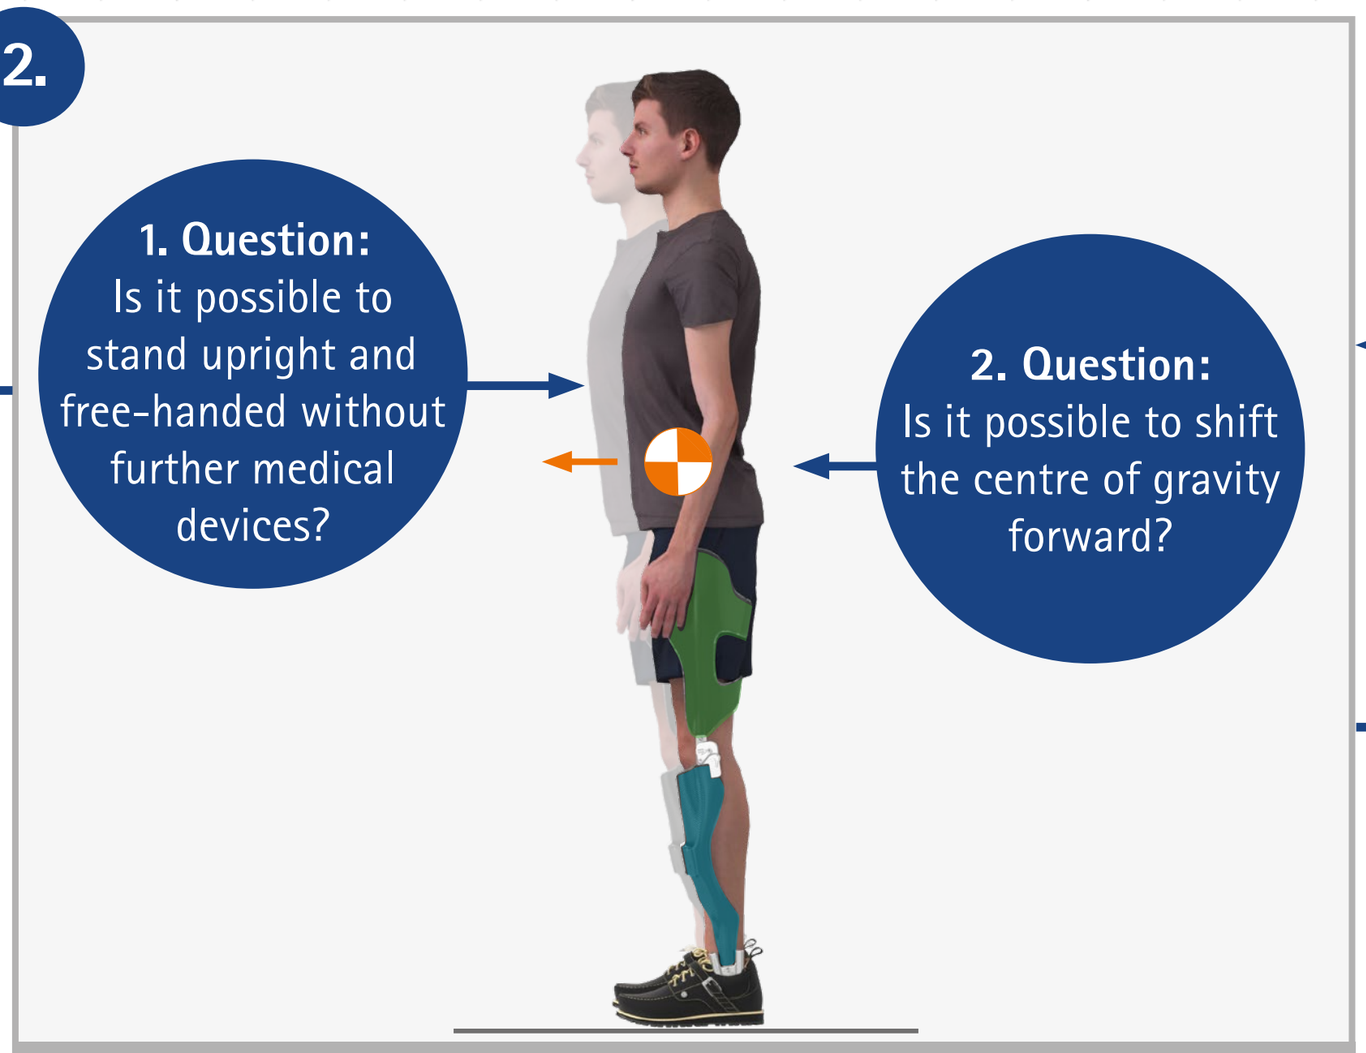

checking the orthosis' alignment statically on the patient

If No, go back to step 1.

If Yes, proceed with step 3.

3.

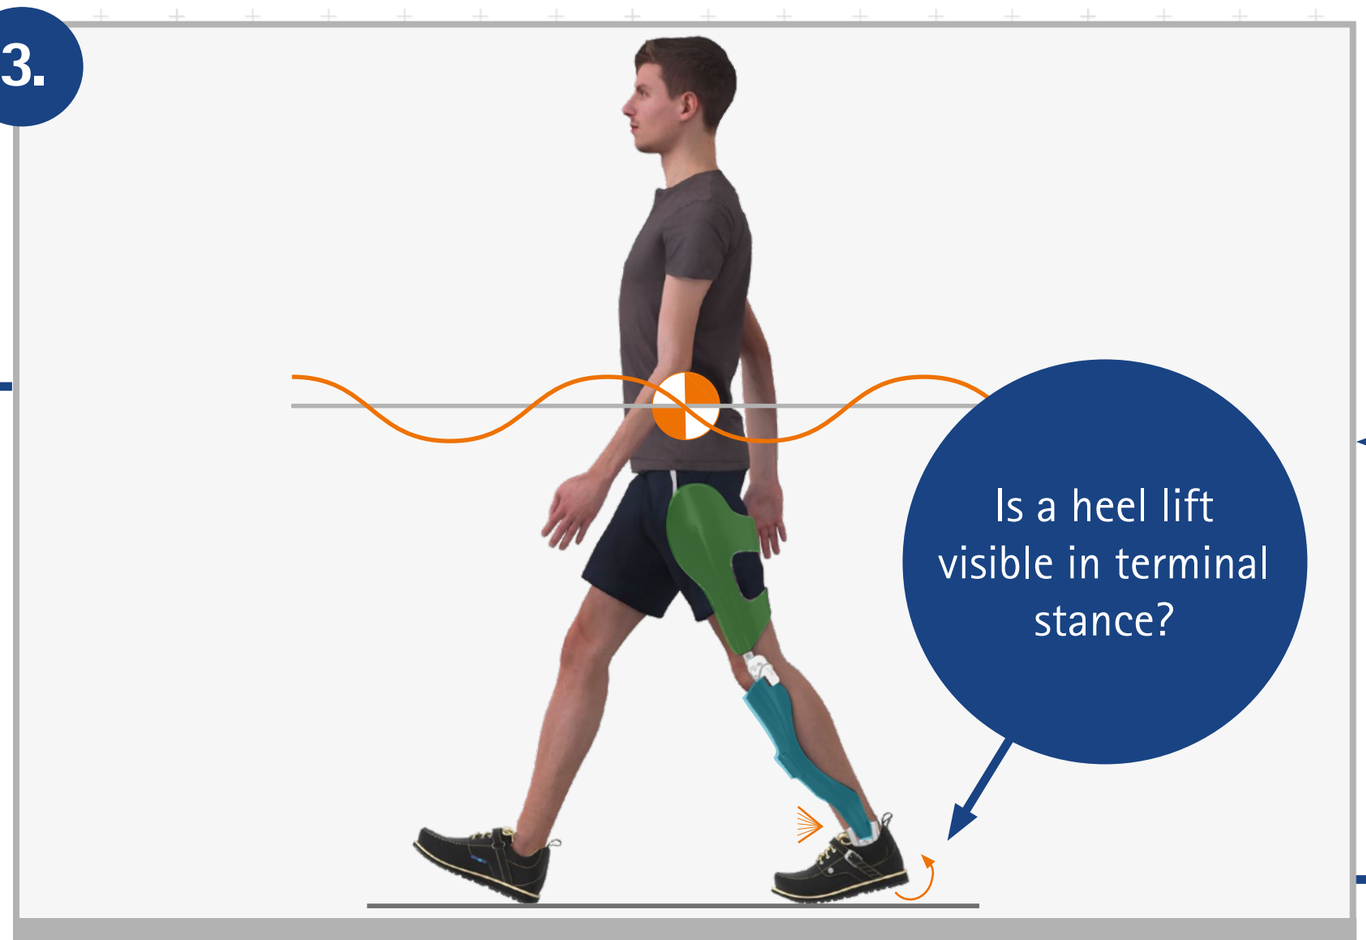

checking the orthosis' alignment dynamically on the patient

If No, go back to step 1.

Yes

You can find further information in the online tutorials.

www.fior-gentz.de/en/online-tutorials

PR2340-DE/GB-2026-03